


Maximus Quick Reference Guide


Does not substitute the official instructions of the Maximus user manual and training guide

Step 1- RF Applicator 2

Warm-Up

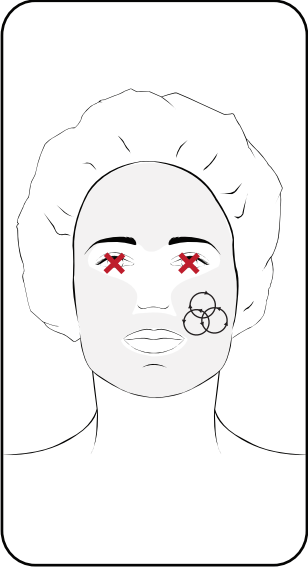

Maintenance

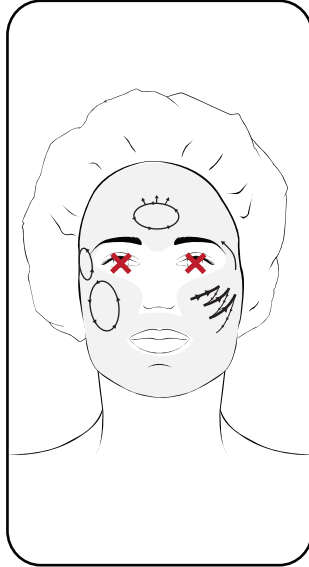


Step 1- RF App. 3

RF only




Step 2- Muscle App. 2

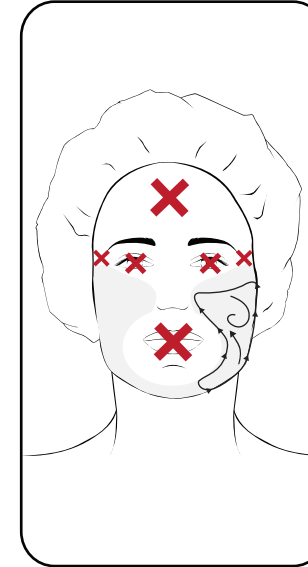


Neck - RF Only

Warm-Up

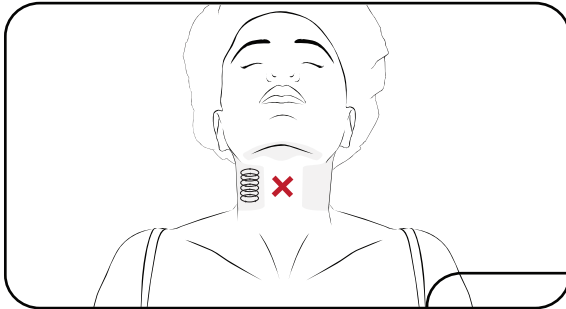

Maintenance

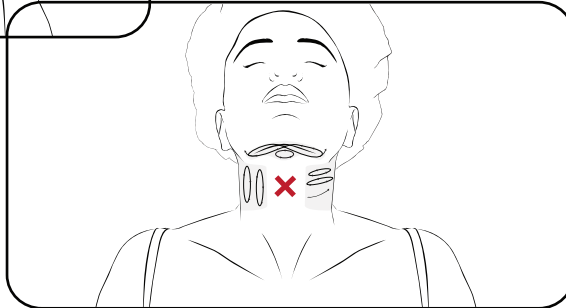

Do not use muscle activation on neck

Avoid Thyroid area.

Face treatment steps:

Step 1: Applicator 2 (Medium applicator), select **FACE (RF only)** and treat full face:

- Warm-up phase: begin with slow circular strokes on one cheek to reach 40-42°C (See illustration).
- Measure surface temperature and after 1-2 minutes and if needed increase RF power by increments of 5.
- Maintenance phase: expand working area to entire half face to reach 40-42°C and maintain temperature. Then repeat on the other side.

Applicator 3 (Small applicator), select **FACE (RF only)** and work on fine lines around eyes and mouth: (See illustration).

Step 2: Applicator 2 (Medium applicator), select **MUSCLE (Dynamic Muscle Activation +low RF (5))** and treat only on cheeks:

- Move applicator slowly on lower cheeks and jaw line from center upwards.
- TriLipo Power default is 10.
- Increase TriLipo Power by 5-10, to patient's tolerance level
- Increase Pulse width by 10-20, to patient's tolerance level
- Increase Frequency to patient's tolerance level

Never treat the area below the eyebrow & never treat over the eye lids & eyeballs.

Avoid temples and forehead.




Maximus Quick Reference Guide


Does not substitute the official instructions of the Maximus user manual and training guide

Arm


Warm-Up

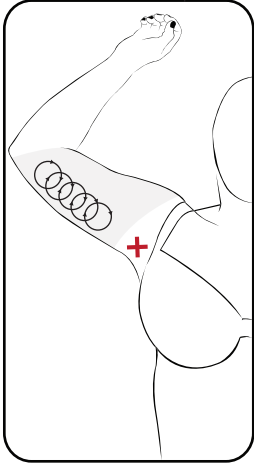


Maintenance

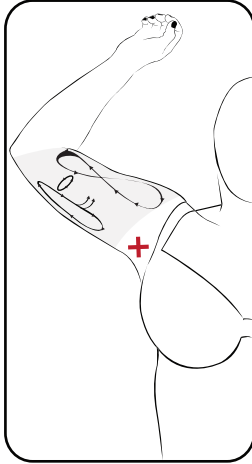

Warm-Up

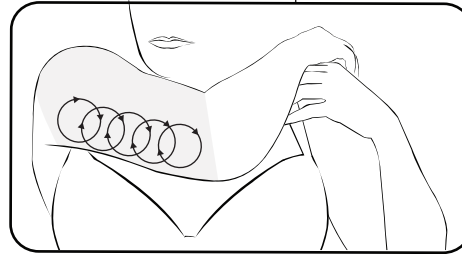


Maintenance

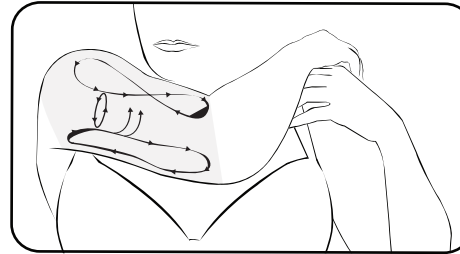


Tummy

Warm-Up

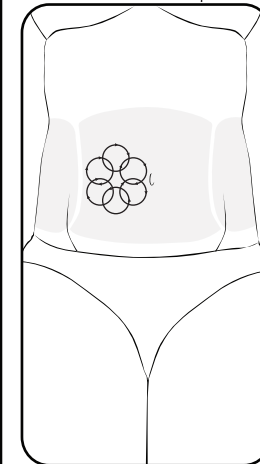

Maintenance

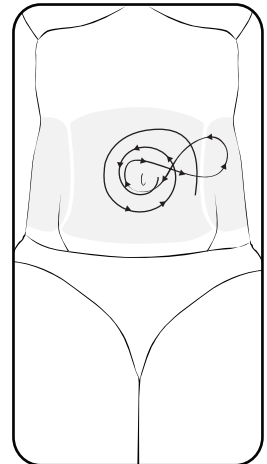

Thighs


Warm-Up




Maintenance



Warm-Up

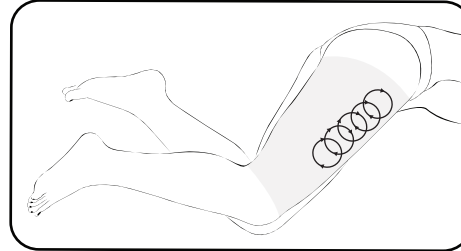


Maintenance

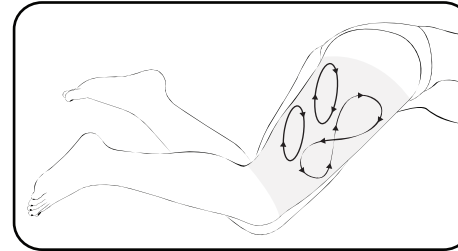


Buttocks

Warm-Up

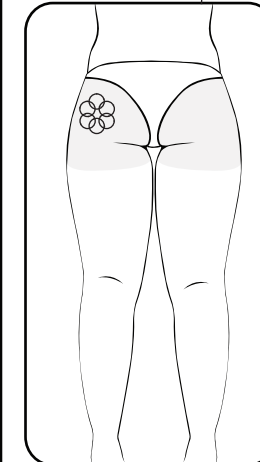

Maintenance

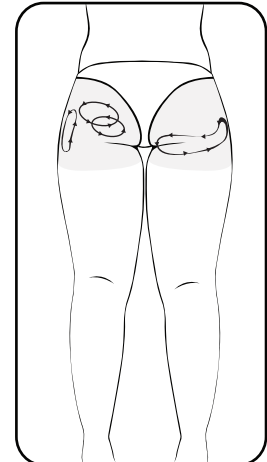

Body Treatment: Applicator 1 or 2*

- Warm up phase is 2-3 minutes – on confined 15x15cm or 10x25cm goal to reach 42°C (do not exceed 45°C)
Increase RF power if needed and work with slow movements
- Maintenance phase: expand working area to include full area being treated and maintain 42°C
- TriLipo Power default is 20.
- Increase TriLipo Power by 5-10, to patient's tolerance level
- Increase Pulse width by 10-20, to patient's tolerance level
- Increase Frequency to patient's tolerance level

* For arms or small/ curved/focal areas use Applicator 2

Avoid the breast, genital and arm pit areas.

